

Review

Image-Guided Transurethral Resection of Bladder Tumors – Current Practice and Future Outlooks

Timothy C. Chang^{a,b,1}, Gautier Marcq^{a,b,1}, Bernhard Kiss^{a,b}, Dharati R. Trivedi^{a,b}, Kathleen E. Mach^{a,b} and Joseph C. Liao^{a,b,*}

^a*Department of Urology, Stanford University School of Medicine, Stanford, CA, USA*

^b*Veterans Affairs Palo Alto Health Care System, Palo Alto, CA, USA*

Abstract. Transurethral resection of bladder tumor (TURBT) under white light cystoscopy (WLC) is the cornerstone for the diagnosis, removal and local staging of non-muscle invasive bladder cancer (NMIBC). Despite technological improvements over the decades, significant shortcomings remain with WLC for tumor detection, thereby impacting the surgical quality and contributing to tumor recurrence and progression. Enhanced cystoscopy modalities such as blue light cystoscopy (BLC) and narrow band imaging (NBI) aid resections by highlighting tumors that might be missed on WLC. Optical biopsy technologies such as confocal laser endomicroscopy (CLE) and optical coherence tomography (OCT) characterize tissue in real-time to ensure a more thorough resection. New resection techniques, particularly en bloc resection, are actively under investigation to improve the overall quality of resections and aid pathologic interpretation. Moreover, new image processing computer algorithms may improve perioperative planning and longitudinal follow-up. Clinical translation of molecular imaging agents is also on the horizon to improve optical diagnosis of bladder cancer. This review focuses on emerging technologies that can impact the quality of TURBT to improve the overall management of NMIBC.

Keywords: Urinary bladder neoplasms, hexaminolevulinic acid, cystoscopy, narrow band imaging, confocal microscopy, computer-assisted, optical coherence tomography, laser surgery, molecular imaging, antigens CD47

INTRODUCTION

Since the first description of endoscopic fulguration of papillary bladder tumors in 1910 [1], transurethral resection of bladder tumor (TURBT) under white light cystoscopy (WLC) has played the central role in bladder cancer diagnosis, removal, and local staging. The goal of TURBT is complete resection of all papillary tumors with concomitant

biopsy of suspicious flat lesions. For non-muscle invasive bladder cancer (NMIBC), high quality TURBT is critical in reducing tumor recurrence and progression [2].

Advances in modern WLC and TURBT include fiber-optic illumination, high definition cameras, and bipolar resection [3]. Nevertheless, significant shortcomings remain including missed tumors, incomplete resection, difficult differentiation of carcinoma *in situ* (CIS) from inflammation, and understaging [4]. In patients undergoing second look TURBT, residual tumors are noted in up to 80% of the surgical specimens within 6 weeks of initial resection [5, 6]. Substantial understaging of high risk bladder cancer

¹These authors contributed equally to this work

*Correspondence to: Joseph C. Liao, 300 Pasteur Dr., Room S-287, Stanford, CA 94305-5118, USA. Tel.: +1 650 852 3284; Fax: +1 650 849 0319; E-mail: jliao@stanford.edu.

Case study

A 60 years old male with a significant history of smoking developed gross hematuria and underwent office cystoscopy as part of workup. A 3 cm papillary tumor was found on the right lateral wall and bladder wash cytology was suspicious. At a later date, monopolar TURBT under WLC was performed under spinal anesthesia and an additional patch of erythema along the posterior bladder was noted and biopsied. During the tumor resection, a significant obturator reflex was triggered and the procedure was terminated. Pathology revealed high grade T1 papillary urothelial carcinoma with muscle present. Biopsy of the erythematous area was inconclusive. Five weeks later, a second look TURBT was performed under general anesthesia. An additional 0.5 cm tumor was found in the right anterior bladder, along with erythematous patches in posterior bladder. The tumor was resected, the erythematous patches biopsied, and deeper resection of the prior resection bed performed. Pathology showed HG T1 cancer, negative resection bed biopsy, and CIS.

Potential benefits of advanced technologies

BLC, NBI or molecular imaging

- *Small papillary tumor found on second TURBT may have been present during the first procedure but not obvious under WLC alone*
- *Inconclusive erythematous patch may have been initially found to be CIS*

CLE

- *May provide adjunctive information on the erythematous lesion for targeting biopsy site with sufficient urothelium for pathological analysis.*

OCT

- *Provide real time assurance of adequate depth of resection*

Bipolar energy

- *May reduce the risk of obturator nerve reflex.*

3D reconstruction and digital bladder mapping

- *Improve perioperative planning and longitudinal follow-up*
- *3D images might indicate if tumor on the second TURBT was initially missed or a recurrence.*

is noted in about 50% of cases when comparing TURBT clinical staging with pathologic staging from cystectomy [7]. Indeed, second look TURBT is recommended for high risk NMIBC after suboptimal initial TURBT, as incomplete resection and understaging have potentially lethal consequences for these patients.

Significant advances in optical imaging technologies and resection techniques have been developed with the goal of assisting surgeons to better identify bladder lesions and improve the quality of TURBT. Enhanced cystoscopy technologies are supported by several prospective trials and meta-analysis [8–10] and included in European Association of Urology (EAU) and American Urology Association (AUA) guidelines for NMIBC [2, 11]. Emerging optical

biopsy technologies hold the promise to significantly augment the precision of TURBT in regards to providing real time tissue characterization. New *en bloc* resection techniques preserve tumor architecture, facilitates better pathological assessment, and potentially offer improved safety profile [12].

The hypothetical case in Box 1 illustrates some of the well-known challenges associated with standard TURBT under WLC, including missed tumors, flat lesion characterization, resection margin assessment, complications of obturator reflex, and pathologic assessment. Here, we review emerging imaging and resection technologies that offer opportunities to significantly enhance TURBT and potentially improve bladder cancer management.

IMPROVING TUMOR DETECTION AND CHARACTERIZATION

Tumor persistence and early recurrence may be due to missed tumors, incomplete resection, reimplantation of tumor cells after resection, and *de novo* tumor formation [13]. CIS is particularly problematic given the challenges of distinguishing CIS from benign bladder lesions leading to a high risk of cancer recurrence and progression.

Blue light cystoscopy (BLC), also known as photodynamic diagnosis or fluorescence cystoscopy, is the most well validated form of enhanced cystoscopy to improve tumor detection [8]. BLC requires preoperative intravesical instillation of hexaminolevulinat (HAL), a photosensitizer that preferentially accumulates in neoplastic cells. Under blue light, red fluorescence is emitted by neoplastic cells (Fig. 1A). A meta-analysis of 2,949 patients revealed 92% sensitivity with BLC for tumor detection compared with 71% with WLC alone [14]. Another meta-analysis of 551 patients showed 87% detection rate for CIS with BLC combined with WLC, whereas WLC alone had 75% detection rate [15]. In addition, under BLC up to 20% more bladder tumors can be detected with a 39% increase in detection of CIS [16]. A prospective, randomized study found a delay in time to tumor

recurrence after BLC-assisted TURBT (16.4 months) compared to WLC alone (9.4 months) [17], and meta-analysis with 634 patients noted a recurrence rate of 34.5% with BLC at 12 months and 45.4% without BLC [8].

Since HAL is not completely cancer-specific, false positive findings associated with BLC can occur [18], particularly in patients with inflammation, recent TURBT, or recent treatment with bacillus Calmette-Guerin (BCG) [19, 20]. The meta-analysis by Mowatt et al. showed that WLC has a higher specificity than BLC (72% vs 57%) [14]. There have been negative studies as well. BLC did not improve the detection rate for patients with known positive cytology in a prospective multicenter randomized trial [21] and other prospective randomized studies did not find improvement on disease recurrence rates with addition of BLC [14, 22, 23]. Weighing the benefit of improved sensitivity in detecting bladder cancer against the drawback of higher false-positive rate, a cost effectiveness study reported that the incorporation of BLC resulted in lower costs over 5 years compared to WLC alone (\$25,921 vs \$30,581, respectively) [24]. In an earlier study looking at BLC with 5-ALA instillation in 191 patients in Germany over 99 months, BLC resulted in €1597 lower cost compared to WLC [25]. A study in Sweden of 2032

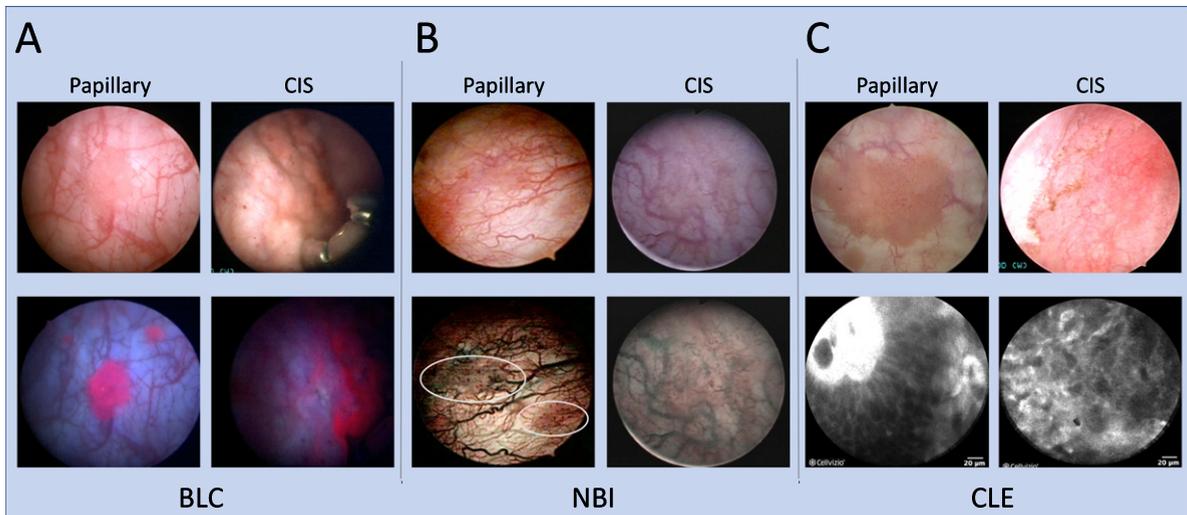


Fig. 1. Imaging modalities for improved bladder tumor detection. Papillary and CIS bladder lesions visualized with BLC, NBI, and CLE with corresponding white light images. (A) Positive, red fluorescence of small, satellite papillary tumors seen on BLC that may be missed on WLC. For CIS, red fluorescence also noted on BLC of what appears to be normal urothelium on WLC. (B) NBI improves visualization of aberrant tumor vasculature. Two papillary tumors are more easily visualized on NBI (encircled). For CIS detection, a patch of erythema is more pronounced under NBI compared to a relatively normal appearing urothelium on WLC. *CIS images for NBI obtained with permission from* [80]. (C) CLE of papillary tumors and CIS provide microscopic detail that can augment macroscopic imaging. A fibrovascular stalk may be visualized as noted in the top left of the papillary CLE example. CIS is notable for a disorganized architecture with pleomorphic cells and indistinct cellular borders.

newly diagnosed bladder cancer patients predicted a total saving of SEK1,321,716 with the use of BLC as an adjunct to WLC, with reduction of 23 cystectomies and 180 TURBTs [26]. While the number of studies calculating cost effectiveness is limited, current data indicates a potential for long term cost savings with the use of BLC.

Under narrow band imaging (NBI), white light is filtered into blue (415 nm) and green (540 nm) wavelengths that are preferentially absorbed by hemoglobin. NBI improves visualization of tumor-associated aberrant mucosal and submucosal vasculature, without the need for exogenous imaging agents (Fig. 1B). NBI has been shown to increase detection of both papillary and flat lesions compared to WLC (94.7% versus 79.2%, respectively) [27], and NBI-assisted TURBT decreased 1-year recurrence compared to standard WLC TURBT (32.9% versus 51.4%, respectively) [28]. A meta-analysis of 1557 patients from six studies found a decreased recurrence rate at 12 months with NBI-assisted TURBT compared to WLC (26% versus 38.6%, respectively) [29]. However, a multicenter randomized trial comparing NBI with standard WLC TURBT revealed no difference in recurrence rates at 1 year follow up (27.1% WLC, 25.4% NBI). It was notable, however, that there was a significant decrease in recurrence in low risk patients (27.3% WLC, 5.6% NBI) [30]. NBI has relatively high false positive rates ranging from 36% to 50% [29, 31, 32], likely related to the subjective nature of image interpretation.

Optical biopsy technologies, which provide high spatial resolution and sub-surface imaging, are complementary to wide field imaging modalities such as WLC, BLC, and NBI. In particular, confocal laser endomicroscopy (CLE) provides micron-scale, histology-like imaging. CLE is FDA approved for application within the urinary tract. For CLE in the bladder, intravesical or intravenous fluorescein is given as the contrast agent and for image acquisition, a fiber-optic probe based on a 488-nm laser is inserted via the working channel of standard cystoscopes and placed in direct contact of the tissue [33–35]. Video sequences (up to 12 hertz) display dynamic imaging of tissue micro-architecture, cellular morphology and vascular flow. Using CLE image criteria described for diagnosis and grading of bladder tumors [36], a study of inter-observer agreement revealed that the sensitivity for discerning cancerous lesions was 89% for urologists using WLC and CLE together [37]. As CIS is often difficult to differentiate from benign flat lesions under WLC, CLE

provides microscopic details (Fig. 1C) to better characterize cellular features that may improve the yield of targeted biopsy. As CLE is probe-based with cross-platform compatibility, it may be combined with WLC and enhanced cystoscopy technologies (BLC and NBI).

High resolution cross-sectional imaging including CT and MRI, as the standard to evaluate the upper urinary tract, has been investigated in pre-TURBT settings for tumor characterization and staging. In a prospective study of 22 patients, Rosenkrantz et al. investigated the accuracy of MRI alone and 18F-FDG simultaneous PET/MRI using a diuresis protocol in bladder cancer patients [38]. PET/MRI increased bladder tumor detection from 77% to 86%, metastatic pelvic lymph nodes detection from 76% to 95% and non-nodal pelvic malignancy to 91% to 100% compared to MRI alone. Further investigation is needed with larger sample sizes to assess the possibility of applying this approach in initial bladder cancer evaluation.

IMPROVING BLADDER TUMOR RESECTION

In addition to better visualization and characterization of tumors and suspicious lesions, adjunctive imaging technologies enhance the technical implementation of TURBT and the completeness of resection. Incomplete resection contributes to understaging of disease that has been noted in up to 50% of patients correlating TURBT-based clinical staging to matched cystectomy specimen [7]. Factors contributing to incomplete TURBT also include decreased visibility due to bleeding and cautery artifacts, and inadequate visualization/differentiation of cancerous tissue at the resection margins.

A key strength of enhanced cystoscopy with BLC and NBI is that the surgeon can toggle back-and-forth between WLC and the enhanced imaging mode, thereby facilitating dynamic implementation during TURBT. This dynamic response allows for real-time assessment of the resection margin. Figure 2A and 2B show resection sites with residual disease identified by BLC and NBI, respectively. Residual tumor that is challenging to detect under WLC may appear to be well delineated compared to the surrounding benign mucosa under BLC as shown in Fig. 2A where the residual BLC enhanced areas correspond to low grade (Patient 1 and 2) and high grade papillary urothelial carcinoma (Patient 3). Future works are needed to

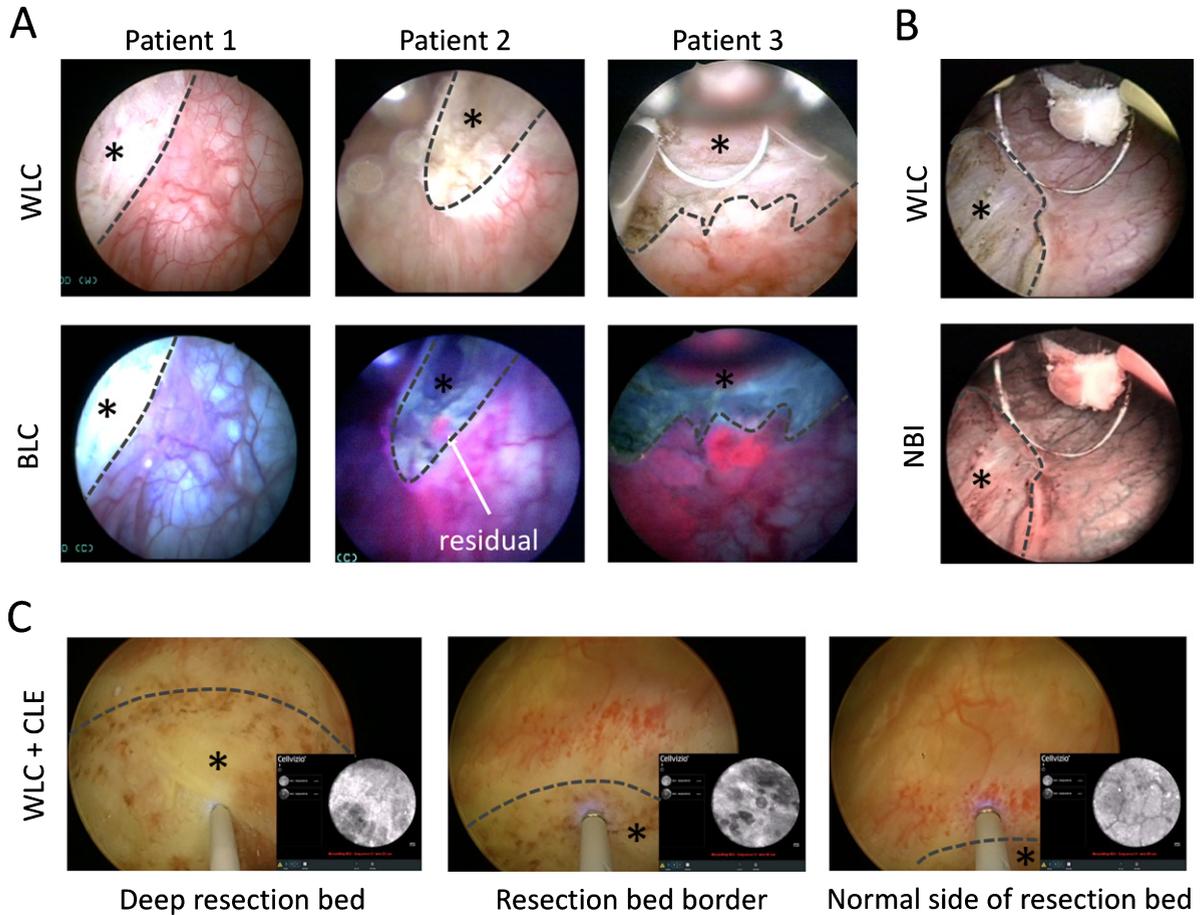


Fig. 2. Imaging of resection bed. (A) BLC can be used to detect residual tumor during TURBT as positive fluorescence is noted at the outside edges of the resection beds in these examples. There are residual tumors noted for patients 2 and 3 even within the resection bed on BLC that is not noted on WLC. (B) Residual tumor at the edge of the resection bed is noted on NBI. *NBI images obtained with permission from [80].* (C) CLE can be used to interrogate the resection bed to determine adequate depth of resection. Features such as elastin strands, muscle fibers and perivesical fat can be visualized in the deep resection bed to verify adequate resection to the muscle layer in real time. All three WLC + CLE images with picture-in-picture are from the same resection bed. In the first image, elastin strands are noted on CLE in the deep resection bed. At the resection bed border, cautery artifact is noted with mostly absence of features seen in the muscle layer. On the normal side of the resection bed, CLE visualizes a capillary network typically seen in normal lamina propria. * – Indicates area within the resection bed. Dashed lines delineate the resection bed border.

determine objectively how enhanced imaging technologies can improve the dynamic aspects of TURBT.

Whereas enhanced cystoscopy technologies are useful to assess the edges of the resection bed, optical biopsy technologies may be utilized to investigate microscopic features of the resection bed, including muscularis propria and perivesical fat [33, 36, 39]. Figure 2C shows an example of using a 0.85 mm CLE imaging probe to interrogate the resection bed, border, and surrounding benign mucosa. Further studies are needed to prospectively determine the clinical utility of resection bed imaging and in combination with enhanced imaging technologies. Nevertheless, this strategy may provide additional confirmation

regarding the depth of resection and residual disease at the time of TURBT.

OCT is another optical biopsy technology that provides mucosal and submucosal imaging in the Z-axis to a depth of 2 mm and spatial resolution of 10 μm , and does not require exogenous contrast agents [40]. A key strength of OCT is the depth of penetration, which enables the possibility of tumor staging. OCT is currently under clinical investigation, with results from several single center studies reported. A single center, retrospective analysis comparing staging by *in vivo* OCT with histopathology revealed 100% sensitivity and 90% specificity in detecting muscle invasive bladder tumors [41], and another single

center prospective study reported 100% sensitivity in detecting invasion of tumors beyond the lamina propria but only 65% overall specificity for bladder tumor detection [40]. Additional studies are needed to determine the suitability of OCT for resection bed imaging.

NEW RESECTION TECHNIQUES

Beyond innovations in imaging modalities, the quality of TURBTs can be improved with advancements in resection techniques. Bipolar, or plasmakinetic, TURBT has emerged in recent years as an alternative to standard monopolar TURBT. The main advantages of bipolar resection include the ability to use isotonic irrigation fluids to decrease the risk of TUR syndrome and potentially improved safety profile compared to monopolar energy [3]. Numerous studies that compared bipolar with monopolar TURBT have found decreased bladder injury associated with obturator nerve reflex [42–44] and improved detrusor sampling [45]. The advantages of bipolar resection may be limited to the safety of the surgical procedure and not clinical outcomes, as most studies find no significant effect of bipolar resection on recurrence rates [42, 46, 47].

Pathological interpretation of TURBT samples are known to be challenging, as resected tumor fragments are subjected to cautery damage, crush artifacts, tangential sections, and lack of spatial orientation caused by random embedding of bladder tissue [12]. *En bloc* resection improves pathological assessment by better preserving tumor architecture and orientation. *En bloc* resection can be performed using standard electrocautery, lasers, or water jet combined with monopolar energy [48]. Laser sources including holmium [49], thulium:YAG [50], and potassium-titanyl-phosphate (green light) [51] have been investigated.

In addition to better preservation of tissue orientation, laser-based *en bloc* resection may reduce surgical morbidity by decreasing bladder perforation through obturator nerve reflex, and post-operative bladder irritation [52]. Impact on cancer-specific outcomes are mixed, as no significant differences in recurrence using *en bloc* resection was noted in 3 prospective studies [53–55], but one small prospective study showed a significant decrease in recurrence (*en bloc* 28.6%, standard TURBT 62.5%) [56]. A multicenter study did not show differences in recurrence between laser (holmium and thulium)

or electrical (monopolar and bipolar) sources [57]. The utility of *en bloc* resection is still under investigation with additional studies needed for validation of cancer-specific outcomes, and standardization of the technique will need to be addressed to facilitate comparison of the various approaches.

PERIOPERATIVE PLANNING AND LONGITUDINAL FOLLOW UP: 3D BLADDER RECONSTRUCTION

Improvements in perioperative care and long term follow up can positively impact bladder cancer management and patient outcomes. Currently, standard documentation of suspicious bladder lesions from cystoscopy, whether in the office or operating room settings, is based on a written description of lesion location, number, size, and morphology. To standardize documentation, the use of a bladder diagram has been advocated in urologic guidelines [2, 58]. Particularly in settings where multiple urologists (e.g. second opinion) are involved in treatment, improved documentation could facilitate communication and follow-up, pre-TURBT surgical planning, and longitudinal surveillance of suspected mucosal lesions. Modern WLC, particularly with the new generation of cameras and videoendoscopes, generates high definition (HD) videos and has enormous data potential. However, WLC is typically used only for real-time guidance and data are not routinely stored.

Recently, a computational method to reconstruct and visualize a 3D model of organs from standard cystoscopic HD videos that captures the shape and surface appearance of the organ has been developed [59]. The algorithm utilizes advanced computer vision techniques and standard cystoscopes for image acquisition (Fig. 3). In contrast to prior efforts [60–62], this algorithm does not require additional hardware. It uses *a priori* data to reconstruct the bladder surface, and presents a complete software-based pipeline to convert the cystoscopic images into a 3D textured model of the bladder. The image preprocessing technique utilizes a structure-from-motion algorithm and the robustness of the reconstruction was tested using tissue-mimicking bladder phantoms. Potential clinical utility was demonstrated using intraoperative cystoscopy videos. Successful reconstruction was achieved for 66.7% of the datasets whereas the definition of successful was that at least 25% of the camera poses could be computed.

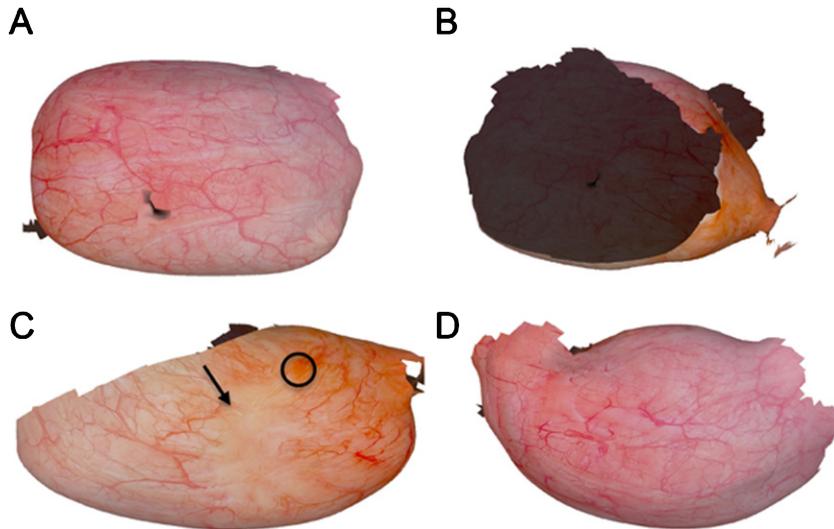


Fig. 3. Reconstruction from a clinical dataset of human bladder. Cystoscopy image reconstruction views from the (A) anterior, (B) posterior, (C) left lateral, and (D) right lateral walls. Black circle and arrow in (C) show regions of a papillary tumor and scarring, respectively. Regions that appear dark represent the interior of the bladder. From [59] with permission.

In a separate 2017 study, image processing and stitching software was used in 12 consecutive whole organ cystoscopies of patients undergoing TURBT to generate panoramic images of the bladders. The authors successfully created HD panoramic images (4096×2048 pixel) in 10 out of 12 cases. However, with this technique there was decreased resolution of the anterior bladder wall as well as low image quality in patients with severe gross hematuria, which interfered with collection of high quality images [63].

Potential applications of these promising 3D reconstruction algorithms include a platform for complete visual medical record of bladder lumen that may be utilized for preoperative surgical planning, cancer surveillance through longitudinal studies of mucosal changes, and trainee or patient education. However, these techniques are at early stage and need further clinical validation. A critical point to consider is that while these emerging technologies provide adjunctive information to standard WLC, timely access to office cystoscopy for hematuria work-up and standard TURBT needs to be prioritized, regardless of the availability of adjunctive imaging technologies [64, 65].

MOLECULAR IMAGE-GUIDED SURGERY – THE FUTURE?

Optical molecular imaging enables the visualization and characterization of biological processes at the molecular level [66, 67]. To improve the

specificity of intraoperative cancer imaging, there is significant interest to develop targeted imaging agents based on fluorescent antibodies, peptides or small molecules. The urinary bladder is an ideal organ for molecular imaging as intravesical application of imaging and therapeutic agents are well established. Through the instillation of molecular imaging agents that bind to specific cancer targets, malignant tumors can be differentiated from benign lesions using endoscopic imaging modalities. The ideal imaging agents would be safe, stable, have appropriate pharmacokinetics, and sensitive and specific for cancer.

For imaging applications, surface antigens are easily accessible for binding to fluorescently labeled antibodies. Although epidermal growth factor (EGFR) and prostate stem cell antigen (PSCA) are potential targets due to contrasting expression patterns between malignant and benign urothelial carcinomas [68–72], they are not ubiquitously expressed on bladder tumors and thus lack the sensitivity needed as imaging targets. CD47, a cell surface protein that is a negative regulator of phagocytosis, is a promising imaging target [73, 74]. CD47 is expressed on the surface of more than 80% of bladder cancer cells but is not expressed on the luminal cells of normal urothelium [74, 75]. Successful *ex vivo* endoscopic imaging of bladder cancer using an anti-CD47 antibody has been reported [75]. Both CLE and BLC were used to detect an intravesically instilled fluorescently tagged antibody

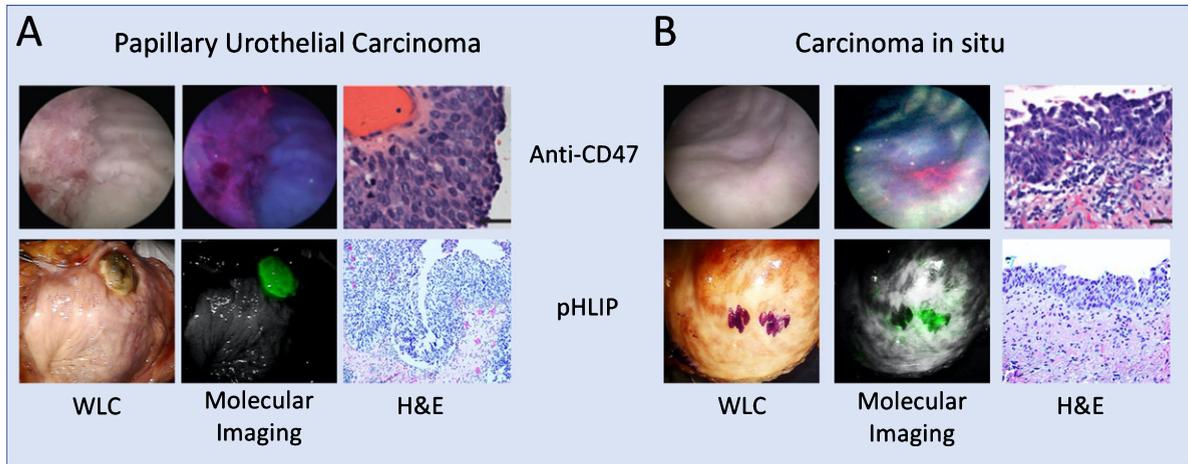


Fig. 4. Molecular imaging of human bladder tumors. *Ex vivo* molecular imaging of human bladder using anti-CD47-Qdot625 (Anti-CD47) imaged with BLC and indocyanine green with pH low insertion peptide (pHLIP) agent imaged with da Vinci Si NIRF imaging system. The respective imaging systems for the two molecular imaging strategies are capable of detecting both (A) papillary tumors and (B) CIS with high sensitivity and specificity. Anti-CD47 images from [75], reprinted with permission from AAAS. pHLIP images obtained from [79] with permission from PNAS.

against human CD47 in *ex vivo* human bladders. BLC imaging of the fluorescent anti-CD47 had 82.9% sensitivity and 90.5% specificity for bladder cancer (Fig. 4).

Small peptides such as pH low insertion peptides (pHLIPs) are a class of membrane-binding peptides that specifically target acidic cells by crossing through the cell membrane in low pH extracellular environments [76, 77]. Tumor cells typically have higher metabolic activity leading to the production of acidic environments [78] that could be targets for pHLIPs. A near infrared fluorescence (NIRF) imaging system was used to image indocyanine green (ICG) conjugated pHLIPs in an *ex vivo* study of radical cystectomy specimen from 22 patients (Fig. 4) [79]. Sensitivity was 97% and specificity was 100% in detecting bladder cancer. However, when necrotic and post-chemotherapy tissue were included, the false positive rate increased and the specificity dropped to 80%. The strategy of developing targeted, specific imaging agents is promising, and further studies are needed to assess *in vivo* performance and toxicity.

The molecular imaging approaches discussed (CD47 and pHLIPs) are in early stages of investigation, and *in vivo* human studies have not been established, pending development of clinical grade labeled antibodies and peptides for *in vivo* human applications. Further investigations are needed before potential application in the clinical setting. However, targeted molecular imaging is a promising avenue

toward improved sensitivity and specificity for cancer detection.

CONCLUSION

The technologies highlighted in this review illustrate the range of technologies at various stages of development aimed at addressing the shortcomings of standard WLC based TURBT. BLC and NBI are recommended in current practice guidelines while molecular imaging of bladder cancer has only been demonstrated to date in *ex vivo* models. As the clinical impact and efficacy of these technologies are validated with further studies, we envision that the future TURBT will harness and combine the advantages of multiple adjunctive technologies to improve the overall quality of TURBT.

ACKNOWLEDGMENTS

GM was funded by Lille 2 University mobility grant. BK was funded by Swiss National Foundation (P300PB_167793/1) and Bern Cancer League.

REFERENCES

- [1] Beer E. Landmark article May 28, 1910: Removal of neoplasms of the urinary bladder. By Edwin Beer. *Jama* 1983;250(10):1324-5.
- [2] Babjuk M, Bohle A, Burger M, Capoun O, Cohen D, Comperat EM, et al. EAU Guidelines on non-muscle-invasive

- urothelial carcinoma of the bladder: Update 2016. *European urology* 2017;71(3):447-61.
- [3] Zainfeld D, Daneshmand S. Transurethral resection of bladder tumors: Improving quality through new techniques and technologies. *Current Urology Reports* 2017;18(5):34.
 - [4] Witjes JA. Bladder carcinoma in situ in 2003: State of the art. *European Urology* 2004;45(2):142-6.
 - [5] Schwaibold HE, Sivalingam S, May F, Hartung R. The value of a second transurethral resection for T1 bladder cancer. *BJU International* 2006;97(6):1199-201.
 - [6] Miladi M, Peyromaure M, Zerbib M, Saighi D, Debre B. The value of a second transurethral resection in evaluating patients with bladder tumours. *European Urology* 2003;43(3):241-5.
 - [7] Cheng L, Neumann RM, Weaver AL, Cheville JC, Leibovich BC, Ramnani DM, et al. Grading and staging of bladder carcinoma in transurethral resection specimens. Correlation with 105 matched cystectomy specimens. *American Journal of Clinical Pathology* 2000;113(2):275-9.
 - [8] Burger M, Grossman HB, Droller M, Schmidbauer J, Herrmann G, Dragoescu O, et al. Photodynamic diagnosis of non-muscle-invasive bladder cancer with hexaminolevulinate cystoscopy: A meta-analysis of detection and recurrence based on raw data. *European Urology* 2013;64(5):846-54.
 - [9] O'Brien T, Ray E, Chatterton K, Khan MS, Chandra A, Thomas K. Prospective randomized trial of hexylaminolevulinate photodynamic-assisted transurethral resection of bladder tumour (TURBT) plus single-shot intravesical mitomycin C vs conventional white-light TURBT plus mitomycin C in newly presenting non-muscle-invasive bladder cancer. *BJU International* 2013;112(8):1096-104.
 - [10] Zheng C, Lv Y, Zhong Q, Wang R, Jiang Q. Narrow band imaging diagnosis of bladder cancer: Systematic review and meta-analysis. *BJU International* 2012;110(11 Pt B):E680-7.
 - [11] Chang SS, Boorjian SA, Chou R, Clark PE, Daneshmand S, Konety BR, et al. Diagnosis and treatment of non-muscle invasive bladder cancer: AUA/SUO guideline. *The Journal of Urology* 2016;196(4):1021-9.
 - [12] Herrmann TR, Wolters M, Kramer MW. Transurethral en bloc resection of nonmuscle invasive bladder cancer: Trend or hype. *Current Opinion in Urology* 2017;27(2):182-90.
 - [13] Van der Heijden AW, JA. Recurrence, Progression, and follow-up in non-muscle-invasive bladder cancer. *European Urology Supplements* 2009;8(7):556-62.
 - [14] Mowatt G, N'Dow J, Vale L, Nabi G, Boachie C, Cook JA, et al. Photodynamic diagnosis of bladder cancer compared with white light cystoscopy: Systematic review and meta-analysis. *Int J Technol Assess Health Care* 2011;27(1):3-10.
 - [15] Lerner SP, Liu H, Wu MF, Thomas YK, Witjes JA. Fluorescence and white light cystoscopy for detection of carcinoma in situ of the urinary bladder. *Urologic Oncology* 2012;30(3):285-9.
 - [16] Kausch I, Sommerauer M, Montorsi F, Stenzl A, Jacqmin D, Jichlinski P, et al. Photodynamic diagnosis in non-muscle-invasive bladder cancer: A systematic review and cumulative analysis of prospective studies. *European Urology* 2010;57(4):595-606.
 - [17] Grossman HB, Stenzl A, Fradet Y, Mynderse LA, Kriegmair M, Witjes JA, et al. Long-term decrease in bladder cancer recurrence with hexaminolevulinate enabled fluorescence cystoscopy. *The Journal of Urology* 2012;188(1):58-62.
 - [18] Stenzl A, Burger M, Fradet Y, Mynderse LA, Soloway MS, Witjes JA, et al. Hexaminolevulinate guided fluorescence cystoscopy reduces recurrence in patients with nonmuscle invasive bladder cancer. *The Journal of Urology* 2010;184(5):1907-13.
 - [19] Lapini A, Minervini A, Masala A, Schips L, Pycha A, Cindolo L, et al. A comparison of hexaminolevulinate (Hexvix((R))) fluorescence cystoscopy and white-light cystoscopy for detection of bladder cancer: Results of the HeRo observational study. *Surgical Endoscopy* 2012;26(12):3634-41.
 - [20] Liu JJ, Droller MJ, Liao JC. New optical imaging technologies for bladder cancer: Considerations and perspectives. *The Journal of Urology* 2012;188(2):361-8.
 - [21] Neuzillet Y, Methorst C, Schneider M, Leuret T, Rouanne M, Radulescu C, et al. Assessment of diagnostic gain with hexaminolevulinate (HAL) in the setting of newly diagnosed non-muscle-invasive bladder cancer with positive results on urine cytology. *Urologic Oncology* 2014;32(8):1135-40.
 - [22] Schumacher MC, Holmang S, Davidsson T, Friedrich B, Pedersen J, Wiklund NP. Transurethral resection of non-muscle-invasive bladder transitional cell cancers with or without 5-aminolevulinic Acid under visible and fluorescent light: Results of a prospective, randomised, multicentre study. *European Urology* 2010;57(2):293-9.
 - [23] Stenzl A, Penkoff H, Dajc-Sommerer E, Zumbraegel A, Hoeltl L, Scholz M, et al. Detection and clinical outcome of urinary bladder cancer with 5-aminolevulinic acid-induced fluorescence cystoscopy: A multicenter randomized, double-blind, placebo-controlled trial. *Cancer* 2011;117(5):938-47.
 - [24] Garfield SS, Gavaghan MB, Armstrong SO, Jones JS. The cost-effectiveness of blue light cystoscopy in bladder cancer detection: United States projections based on clinical data showing 4.5 years of follow up after a single hexaminolevulinate hydrochloride instillation. *The Canadian Journal of Urology* 2013;20(2):6682-9.
 - [25] Otto W, Burger M, Fritsche HM, Blana A, Roessler W, Knuechel R, et al. Photodynamic diagnosis for superficial bladder cancer: Do all risk-groups profit equally from oncological and economic long-term results? *Clin Med Oncol* 2009;3:53-8.
 - [26] Malmstrom PU, Hedelin H, Thomas YK, Thompson GJ, Durrant H, Furniss J. Fluorescence-guided transurethral resection of bladder cancer using hexaminolevulinate: Analysis of health economic impact in Sweden. *Scand J Urol Nephrol* 2009;43(3):192-8.
 - [27] Cauberg EC, Kloen S, Visser M, de la Rosette JJ, Babjuk M, Soukup V, et al. Narrow band imaging cystoscopy improves the detection of non-muscle-invasive bladder cancer. *Urology* 2010;76(3):658-63.
 - [28] Naselli A, Introini C, Timossi L, Spina B, Fontana V, Pezzi R, et al. A randomized prospective trial to assess the impact of transurethral resection in narrow band imaging modality on non-muscle-invasive bladder cancer recurrence. *European Urology* 2012;61(5):908-13.
 - [29] Xiong Y, Li J, Ma S, Ge J, Zhou L, Li D, et al. A meta-analysis of narrow band imaging for the diagnosis and therapeutic outcome of non-muscle invasive bladder cancer. *PLoS One* 2017;12(2):e0170819.
 - [30] Naito S, Algaba F, Babjuk M, Bryan RT, Sun YH, Valiquette L, et al. The Clinical Research Office of the Endourological Society (CROES) Multicentre randomised trial of narrow

- band imaging-assisted transurethral resection of bladder tumour (TURBT) Versus conventional white light imaging-assisted TURBT in primary non-muscle-invasive bladder cancer patients: Trial protocol and 1-year results. *European Urology* 2016;70(3):506-15.
- [31] Ye Z, Hu J, Song X, Li F, Zhao X, Chen S, et al. A comparison of NBI and WLI cystoscopy in detecting non-muscle-invasive bladder cancer: A prospective, randomized and multi-center study. *Scientific Reports* 2015;5:10905.
- [32] Herr HW, Donat SM. A comparison of white-light cystoscopy and narrow-band imaging cystoscopy to detect bladder tumour recurrences. *BJU International* 2008;102(9):1111-4.
- [33] Chen SP, Liao JC. Confocal laser endomicroscopy of bladder and upper tract urothelial carcinoma: A new era of optical diagnosis? *Current Urology Reports* 2014;15(9):437.
- [34] Jabbour JM, Saldua MA, Bixler JN, Maitland KC. Confocal endomicroscopy: Instrumentation and medical applications. *Ann Biomed Eng* 2012;40(2):378-97.
- [35] Chang TC, Liu JJ, Liao JC. Probe-based confocal laser endomicroscopy of the urinary tract: The technique. *Journal of Visualized Experiments: JoVE* 2013(71):e4409.
- [36] Wu K, Liu JJ, Adams W, Sonn GA, Mach KE, Pan Y, et al. Dynamic real-time microscopy of the urinary tract using confocal laser endomicroscopy. *Urology* 2011;78(1):225-31.
- [37] Chang TC, Liu JJ, Hsiao ST, Pan Y, Mach KE, Lepert JT, et al. Interobserver agreement of confocal laser endomicroscopy for bladder cancer. *Journal of Endourology* 2013;27(5):598-603.
- [38] Rosenkrantz AB, Friedman KP, Ponzio F, Raad RA, Jackson K, Huang WC, et al. Prospective pilot study to evaluate the incremental value of PET information in patients with bladder cancer undergoing 18F-FDG simultaneous PET/MRI. *Clin Nucl Med* 2017;42(1):e8-e15.
- [39] Sonn GA, Jones SN, Tarin TV, Du CB, Mach KE, Jensen KC, et al. Optical biopsy of human bladder neoplasia with in vivo confocal laser endomicroscopy. *The Journal of Urology* 2009;182(4):1299-305.
- [40] Karl A, Stepp H, Willmann E, Buchner A, Hocaoglu Y, Stief C, et al. Optical coherence tomography for bladder cancer – ready as a surrogate for optical biopsy? Results of a prospective mono-centre study. *European Journal of Medical Research* 2010;15(3):131-4.
- [41] Goh AC, Tresser NJ, Shen SS, Lerner SP. Optical coherence tomography as an adjunct to white light cystoscopy for intravesical real-time imaging and staging of bladder cancer. *Urology* 2008;72(1):133-7.
- [42] Xishuang S, Deyong Y, Xiangyu C, Tao J, Quanlin L, Hongwei G, et al. Comparing the safety and efficiency of conventional monopolar, plasmakinetic, and holmium laser transurethral resection of primary non-muscle invasive bladder cancer. *Journal of Endourology* 2010;24(1):69-73.
- [43] Bolat D, Gunlusoy B, Degirmenci T, Ceylan Y, Polat S, Aydin E, et al. Comparing the short-term outcomes and complications of monopolar and bipolar transurethral resection of non-muscle invasive bladder cancers: A prospective, randomized, controlled study. *Arch Esp Urol* 2016;69(5):225-33.
- [44] Zhao C, Tang K, Yang H, Xia D, Chen Z. Bipolar versus monopolar transurethral resection of nonmuscle-invasive bladder cancer: A meta-analysis. *Journal of Endourology* 2016;30(1):5-12.
- [45] Teoh JY, Chan ES, Yip SY, Tam HM, Chiu PK, Yee CH, et al. Comparison of Detrusor muscle sampling rate in monopolar and bipolar transurethral resection of bladder tumor: A randomized trial. *Annals of Surgical Oncology* 2017;24(5):1428-34.
- [46] Del Rosso A, Pace G, Masciovecchio S, Saldutto P, Galatioto GP, Vicentini C. Plasmakinetic bipolar versus monopolar transurethral resection of non-muscle invasive bladder cancer: A single center randomized controlled trial. *International Journal of Urology: Official Journal of the Japanese Urological Association* 2013;20(4):399-403.
- [47] Cui Y, Chen H, Liu L, Chen J, Qi L, Zu X. Comparing the efficiency and safety of bipolar and monopolar transurethral resection for non-muscle invasive bladder tumors: A systematic review and meta-analysis. *J Laparoendosc Adv Surg Tech A* 2016;26(3):196-202.
- [48] Nagele U, Kugler M, Nicklas A, Merseburger AS, Walcher U, Mikuz G, et al. Waterjet hydrodissection: First experiences and short-term outcomes of a novel approach to bladder tumor resection. *World J Urol* 2011;29(4):423-7.
- [49] Das A, Gilling P, Fraundorfer M. Holmium laser resection of bladder tumors (HoLRBT). *Tech Urol* 1998;4(1):12-4.
- [50] Wolters M, Kramer MW, Becker JU, Christgen M, Nagele U, Imkamp F, et al. Tm:YAG laser en bloc mucosectomy for accurate staging of primary bladder cancer: Early experience. *World J Urol* 2011;29(4):429-32.
- [51] He D, Fan J, Wu K, Wang X, Wu D, Li L, et al. Novel green-light KTP laser en bloc enucleation for nonmuscle-invasive bladder cancer: Technique and initial clinical experience. *Journal of Endourology* 2014;28(8):975-9.
- [52] D'Souza N, Verma A. Holmium laser transurethral resection of bladder tumor: Our experience. *Urology Annals* 2016;8(4):439-43.
- [53] Chen J, Zhao Y, Wang S, Jin X, Sun P, Zhang L, et al. Green-light laser en bloc resection for primary non-muscle-invasive bladder tumor versus transurethral electroresection: A prospective, nonrandomized two-center trial with 36-month follow-up. *Lasers in Surgery and Medicine* 2016;48(9):859-65.
- [54] Chen X, Liao J, Chen L, Qiu S, Mo C, Mao X, et al. En bloc transurethral resection with 2-micron continuous-wave laser for primary non-muscle-invasive bladder cancer: A randomized controlled trial. *World J Urol* 2015;33(7):989-95.
- [55] Liu H, Wu J, Xue S, Zhang Q, Ruan Y, Sun X, et al. Comparison of the safety and efficacy of conventional monopolar and 2-micron laser transurethral resection in the management of multiple nonmuscle-invasive bladder cancer. *The Journal of International Medical Research* 2013;41(4):984-92.
- [56] Sureka SK, Agarwal V, Agnihotri S, Kapoor R, Srivastava A, Mandhani A. Is en-bloc transurethral resection of bladder tumor for non-muscle invasive bladder carcinoma better than conventional technique in terms of recurrence and progression?: A prospective study. *Indian Journal of Urology: IJU: Journal of the Urological Society of India* 2014;30(2):144-9.
- [57] Kramer MW, Rassweiler JJ, Klein J, Martov A, Baykov N, Lusuardi L, et al. En bloc resection of urothelium carcinoma of the bladder (EBRUC): A European multicenter study to compare safety, efficacy, and outcome of laser and electrical en bloc transurethral resection of bladder tumor. *World J Urol* 2015;33(12):1937-43.

- [58] Mariappan P, Rai B, El-Mokadem I, Anderson CH, Lee H, Stewart S, et al. Real-life experience: Early recurrence with hexvix photodynamic diagnosis-assisted transurethral resection of bladder tumour vs good-quality white light TURBT in new non-muscle-invasive bladder cancer. *Urology* 2015;86(2):327-31.
- [59] Lurie KL, Angst R, Zlatev DV, Liao JC, Ellerbee Bowden AK. 3D reconstruction of cystoscopy videos for comprehensive bladder records. *Biomedical Optics Express* 2017;8(4):2106-23.
- [60] Soper TD, Porter MP, Seibel EJ. Surface mosaics of the bladder reconstructed from endoscopic video for automated surveillance. *IEEE Transactions on Bio-Medical Engineering* 2012;59(6):1670-80.
- [61] Penne J, Holler K, Sturmer M, Schrauder T, Schneider A, Engelbrecht R, et al. Time-of-Flight 3-D endoscopy. *Med Image Comput Assist Interv* 2009;12(Pt 1):467-74.
- [62] Agenant M, Noordmans HJ, Koomen W, Bosch JL. Real-time bladder lesion registration and navigation: A phantom study. *PLoS One* 2013;8(1):e54348.
- [63] Kriegmair MC, Bergen T, Ritter M, Mandel P, Michel MS, Wittenberg T, et al. Digital mapping of the urinary bladder: Potential for standardized cystoscopy reports. *Urology* 2017;104:235-41.
- [64] Ngo B, Papa N, Perera M, Bolton D, Sengupta S. Predictors of delay to cystoscopy and adequacy of investigations in patients with haematuria. *BJU International* 2017;119(Suppl 5):19-25.
- [65] Ngo B, Perera M, Papa N, Bolton D, Sengupta S. Factors affecting the timeliness and adequacy of haematuria assessment in bladder cancer: A systematic review. *BJU International* 2017;119(Suppl 5):10-8.
- [66] Greco F, Cadeddu JA, Gill IS, Kaouk JH, Remzi M, Thompson RH, et al. Current perspectives in the use of molecular imaging to target surgical treatments for genitourinary cancers. *European Urology* 2014;65(5):947-64.
- [67] Zlatev DV, Altobelli E, Liao JC. Advances in imaging technologies in the evaluation of high-grade bladder cancer. *The Urologic clinics of North America* 2015;42(2):147-57, vii.
- [68] Pfost B, Seidl C, Autenrieth M, Saur D, Bruchertseifer F, Morgenstern A, et al. Intravesical alpha-radioimmunotherapy with ²¹³Bi-anti-EGFR-mAb defeats human bladder carcinoma in xenografted nude mice. *J Nucl Med* 2009;50(10):1700-8.
- [69] Mazzucchelli R, Barbisan F, Santinelli A, Lopez-Beltran A, Cheng L, Scarpelli M, et al. Immunohistochemical expression of prostate stem cell antigen in cystoprostatectomies with incidental prostate cancer. *International Journal of Immunopathology and Pharmacology* 2009;22(3):755-62.
- [70] Lepin EJ, Leyton JV, Zhou Y, Olafsen T, Salazar FB, McCabe KE, et al. An affinity matured minibody for PET imaging of prostate stem cell antigen (PSCA)-expressing tumors. *European Journal of Nuclear Medicine and Molecular Imaging* 2010;37(8):1529-38.
- [71] Carlsson J. Potential for clinical radionuclide-based imaging and therapy of common cancers expressing EGFR-family receptors. *Tumour Biology: The Journal of the International Society for Oncodevelopmental Biology and Medicine* 2012;33(3):653-9.
- [72] Amara N, Palapattu GS, Schrage M, Gu Z, Thomas GV, Dorey F, et al. Prostate stem cell antigen is overexpressed in human transitional cell carcinoma. *Cancer Research* 2001;61(12):4660-5.
- [73] Willingham SB, Volkmer JP, Gentles AJ, Sahoo D, Dalerba P, Mitra SS, et al. The CD47-signal regulatory protein alpha (SIRPα) interaction is a therapeutic target for human solid tumors. *Proceedings of the National Academy of Sciences of the United States of America* 2012;109(17):6662-7.
- [74] Chan KS, Espinosa I, Chao M, Wong D, Ailles L, Diehn M, et al. Identification, molecular characterization, clinical prognosis, and therapeutic targeting of human bladder tumor-initiating cells. *Proceedings of the National Academy of Sciences of the United States of America* 2009;106(33):14016-21.
- [75] Pan Y, Volkmer JP, Mach KE, Rouse RV, Liu JJ, Sahoo D, et al. Endoscopic molecular imaging of human bladder cancer using a CD47 antibody. *Science Translational Medicine* 2014;6(260):260ra148.
- [76] Andreev OA, Engelman DM, Reshetnyak YK. Targeting diseased tissues by pHLIP insertion at low cell surface pH. *Frontiers in Physiology* 2014;5:97.
- [77] Weerakkody D, Moshnikova A, Thakur MS, Moshnikova V, Daniels J, Engelman DM, et al. Family of pH (low) insertion peptides for tumor targeting. *Proceedings of the National Academy of Sciences of the United States of America* 2013;110(15):5834-9.
- [78] Bailey KM, Wojtkowiak JW, Hashim AI, Gillies RJ. Targeting the metabolic microenvironment of tumors. *Advances in Pharmacology (San Diego, Calif)* 2012;65:63-107.
- [79] Golijanin J, Amin A, Moshnikova A, Brito JM, Tran TY, Adochite RC, et al. Targeted imaging of urothelium carcinoma in human bladders by an ICG pHLIP peptide ex vivo. *Proceedings of the National Academy of Sciences of the United States of America* 2016;113(42):11829-34.
- [80] Jecu M, Geavlete B, Multescu R, Stanescu F, Moldoveanu C, Adou L, et al. NBI cystoscopy in routine urological practice – from better vision to improve therapeutic management. *J Med Life* 2014;7(2):282-6.